

AD-A083 875

AD A 083 875

USADAC TECHNICAL LIBRARY



5 0712 01017139 4

AD

TECHNICAL REPORT ARBRL-TR-02213

SIX CHANNEL DIGITAL DELAY GENERATOR

Clifford L. Aseltine

TECHNICAL
LIBRARY

January 1980



US ARMY ARMAMENT RESEARCH AND DEVELOPMENT COMMAND
BALLISTIC RESEARCH LABORATORY
ABERDEEN PROVING GROUND, MARYLAND

Approved for public release; distribution unlimited.

Destroy this report when it is no longer needed.
Do not return it to the originator.

Secondary distribution of this report by originating
or sponsoring activity is prohibited.

Additional copies of this report may be obtained
from the National Technical Information Service,
U.S. Department of Commerce, Springfield, Virginia
22151.

The findings in this report are not to be construed as
an official Department of the Army position, unless
so designated by other authorized documents.

*The use of trade names or manufacturers' names in this report
does not constitute indorsement of any commercial product.*

UNCLASSIFIED

SECURITY CLASSIFICATION OF THIS PAGE (When Data Entered)

REPORT DOCUMENTATION PAGE		READ INSTRUCTIONS BEFORE COMPLETING FORM
1. REPORT NUMBER TECHNICAL REPORT ARBRL-TR-02213	2. GOVT ACCESSION NO.	3. RECIPIENT'S CATALOG NUMBER
4. TITLE (and Subtitle) SIX CHANNEL DIGITAL DELAY GENERATOR		5. TYPE OF REPORT & PERIOD COVERED Final
		6. PERFORMING ORG. REPORT NUMBER
7. AUTHOR(s) Clifford L. Aseltine		8. CONTRACT OR GRANT NUMBER(s)
9. PERFORMING ORGANIZATION NAME AND ADDRESS US Army Ballistic Research Laboratory (ATTN: DRDAR-BLT) Aberdeen Proving Ground, MD 21005		10. PROGRAM ELEMENT, PROJECT, TASK AREA & WORK UNIT NUMBERS 1L161101A91A
11. CONTROLLING OFFICE NAME AND ADDRESS US Army Armament Research & Development Command US Army Ballistic Research Laboratory (ATTN: DRDAR-BL) Aberdeen Proving Ground, MD 21005		12. REPORT DATE JANUARY 1980
		13. NUMBER OF PAGES 19
14. MONITORING AGENCY NAME & ADDRESS (if different from Controlling Office)		15. SECURITY CLASS. (of this report) UNCLASSIFIED
		15a. DECLASSIFICATION/DOWNGRADING SCHEDULE
16. DISTRIBUTION STATEMENT (of this Report) Approved for public release, distribution unlimited.		
17. DISTRIBUTION STATEMENT (of the abstract entered in Block 20, if different from Report)		
18. SUPPLEMENTARY NOTES		
19. KEY WORDS (Continue on reverse side if necessary and identify by block number) delay generator, flash x-ray, digital delay generator <i>Pulse</i> <i>7000 2400</i>		
20. ABSTRACT (Continue on reverse side if necessary and identify by block number) (dlc) A six channel digital delay generator is described which can provide delays of .5 μ sec to 10,000 μ sec. Delays are digitally generated and are designed to operate in high RFI areas such as those encountered in ballistic measurements.		

TABLE OF CONTENTS

	Page
LIST OF ILLUSTRATIONS	5
I. INTRODUCTION	7
II. CONCEPT	7
III. DESIGN AND CONSTRUCTION	10
DISTRIBUTION LIST	19

LIST OF ILLUSTRATIONS

Figure	Page
1. Block Diagram of a Digital Delay Generator	8
2. Tektronix DD501 Events Counter	9
3. Schematic Diagram of Clock Circuit and Cable Driver	11
4. Oscillator Circuit Board (A) Component Side (B) Circuit Side	12
5. Schematic Diagram of Pulse Shaper and Output Driver	13
6. Pulse Shaper and Output Driver Circuit Board	15
7. DD501 Events Counter with Pulse Shaper and Output Driver Board Installed	16
8. Photograph of Completed Six Channel Delay System . . .	14

I. INTRODUCTION

In ballistic measurements, considerable use is made of delay units having time period ranges spanning .5 μ sec to 100 μ sec or more. Historically, delays were generated by R-C networks that fired thyratrons to provide the required output pulses. Because of severe electrical interference, very high input level (30-200 volts) signals were required to prevent false triggering. With the widespread use of digital techniques, time delays with reproducibilities better than .1 μ sec are now available. Besides reproducibility, digital techniques require far less set up time and reduce chances of error. Therefore, since reproducibility and efficiency were prime concerns, digital delay techniques were chosen as the most desirable for our program.

II. CONCEPT

The basic concept of a digital delay system is quite simple. Figure 1 shows a simplified block diagram. A digital counter, upon command from the start control, counts the clock pulses until a predetermined number of pulses that has been set by the delay switches has been counted. At this time, an output pulse is generated that signifies the end of the delay period. This pulse can then be shaped to match the requirement of the peripheral equipment. The clock frequency can then be selected to provide the maximum time delay that might be selected by the switches. A chief advantage of this system is its inherent low sensitivity to interference from RFI generated by explosive firing units with spark gap initiators. A single pulse from an external noise source will only shorten the time delay by one clock pulse if this pulse occurs between two clock pulses. It was decided to use existing event counters manufactured by Tektronix as the delay generators. This unit was chosen because of the elaborate input discrimination and pulse shaping networks and because six units could be contained in one 483 mm rack width. Figure 2 shows a picture of the Tektronix DD501 events counter. The front panel delay switches allow up to a 100,000 clock pulse delay before providing an output pulse. All clock pulse and input trigger levels can be permanently set by screw driver adjustments or overridden by manual front panel controls. The input parameters of 1 meg ohm/20 pf allow the use of make and break screens for remote starting of the delay. For more detailed specifications, see the DD501 instruction manual.

The system clock was an M. F. electronics model 5401-1 in a printed circuit mounting package. This particular model has a 10 MHz temperature compensated crystal oscillator with a screwdriver adjustment for frequency correction.

The output circuits were designed and constructed in-house to provide the high voltages required to trip flash x-ray systems and thyatron controlled firing units. Details of this circuit are described in the next section.

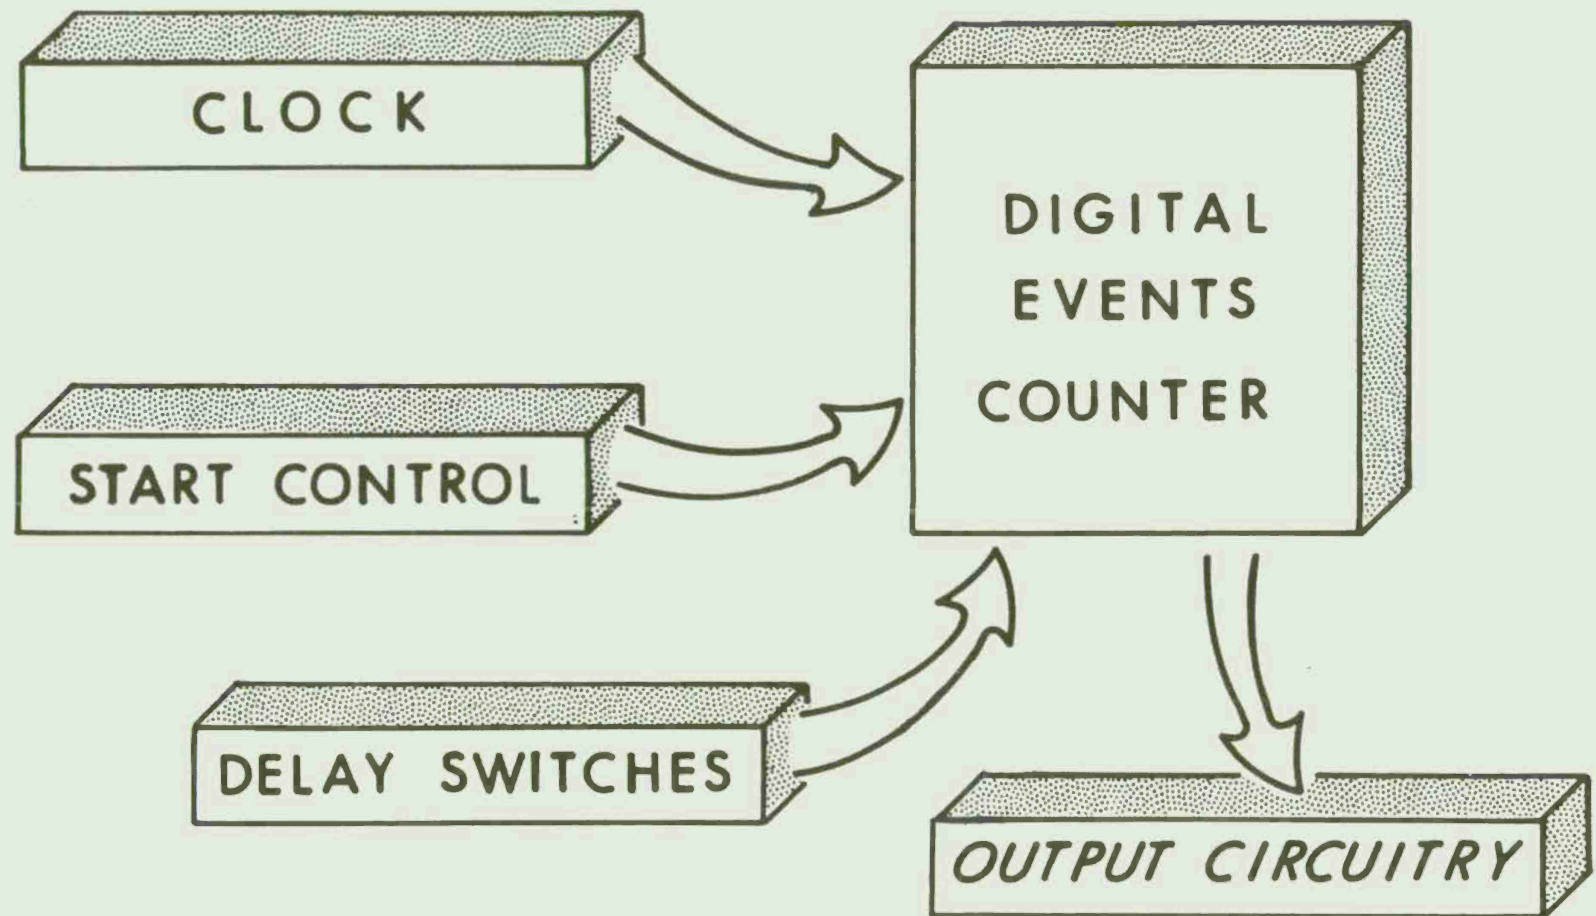


Figure 1. Block Diagram of a Digital Delay Generator

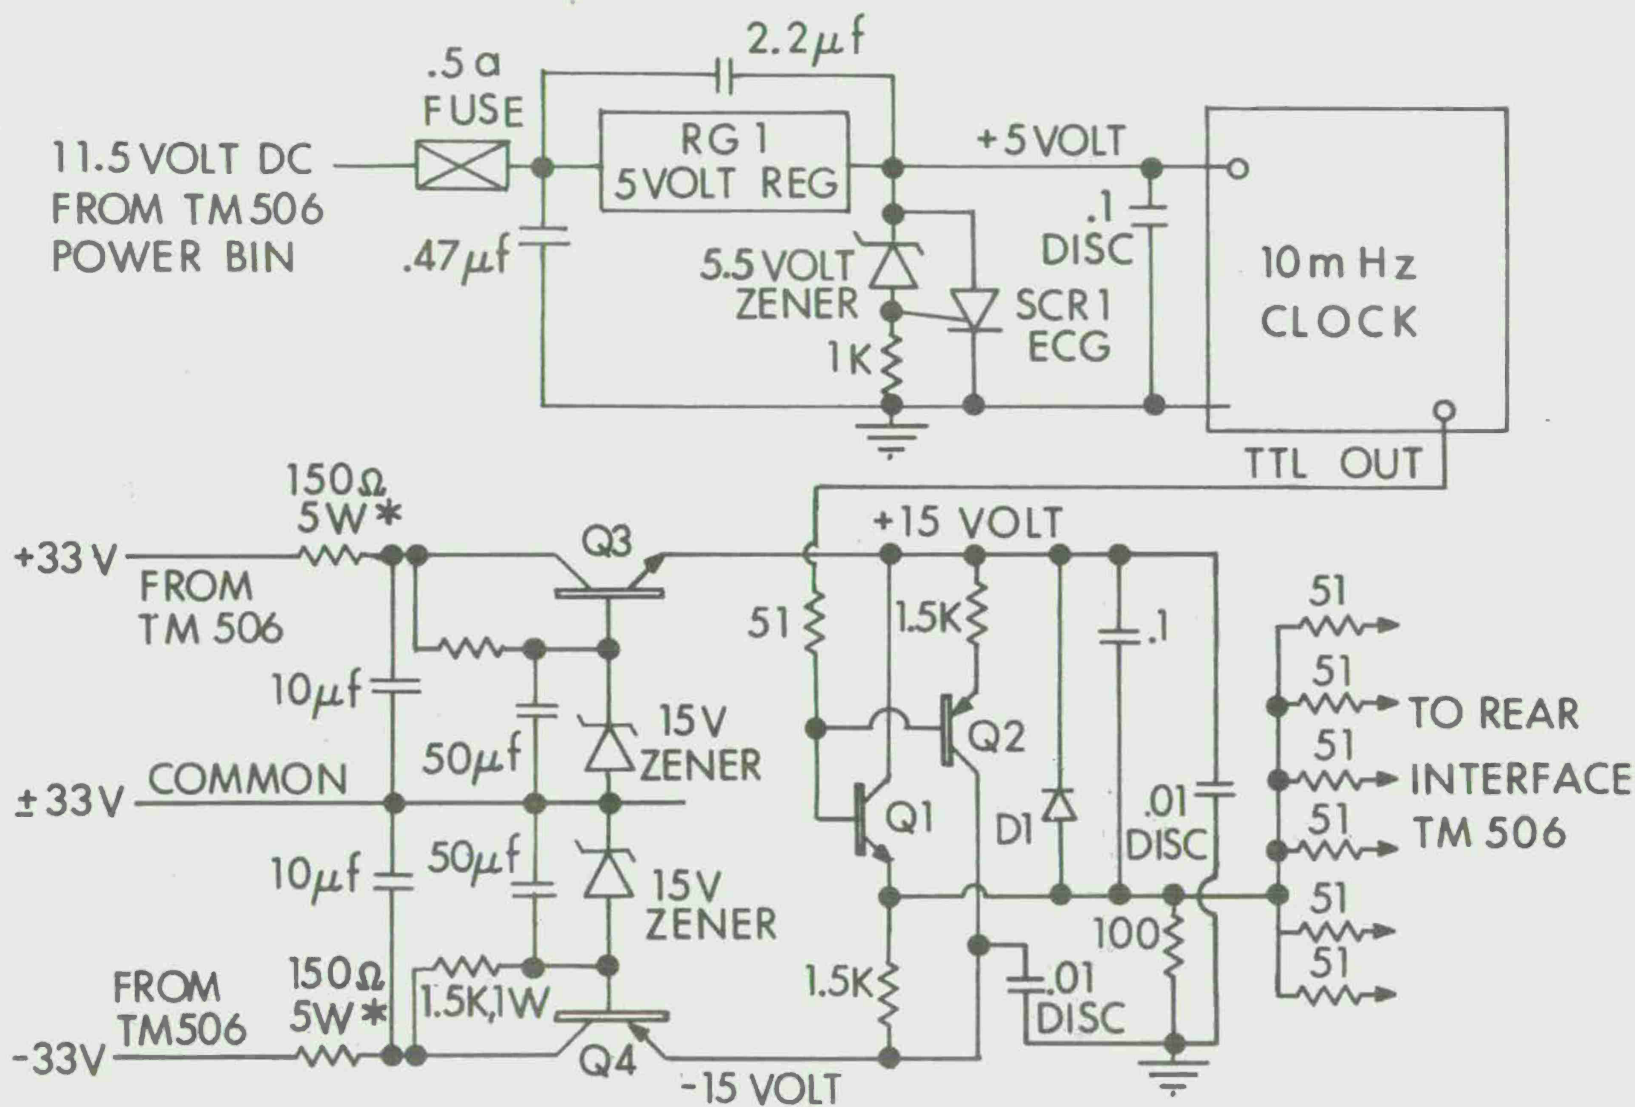


Figure 2. Tektronix DD501 Events Counter

III. DESIGN AND CONSTRUCTION

The circuit diagrams for the crystal clock oscillator, cable driver, and their required power supplies are shown in Figure 3. The 5 volt supply for the clock is obtained from a monolithic regulator, RG1. SCR1 is used as a clamp to short the 5 volt line to ground in case of regulator failure. The clock output is TTL compatible and not capable of driving six 50 ohm lines to the events inputs of the DD501's. The switching transistors Q_1 and Q_2 supply the proper impedance transformation to drive the 50 ohm cables. The disc capacitors on the 5 and ± 15 volt lines are required to reduce internal ringing problems related to the fast TTL pulses. After considerable experimentation, the output resistances consisting of six 51 ohm and one 100 ohm resistors were found to provide the optimum signal at the other end of the 50 ohm cable that was terminated only by the 1 meg/20 pf of the events input. The events input compensation capacitor can be set if required to reduce any remaining ring observed at the events input jack. The ± 15 volts supplies are of a straight forward design. The only unusual portion is the addition of two 10 μ farad capacitors after the 150 Ω resistors. These are mounted on the clock board and are required to decouple the clock board itself from the TM506 mainframe.

Figure 4(a) and 4(b) show the physical layout of the clock circuit card. The layout of the power supplies was not critical except for the two 150 Ω /5 watt resistors that are mounted on the TM506 interface board. However, the layout of the line driver, Figure 4(b), was important in order to reduce ringing. Figure 4(b) shows the layout of the circuitry around Q_1 and Q_2 . Wiring lengths are kept to a minimum by mounting the two transistors and their components right over the output pin of the oscillator. The heat sink fins of the transistors are bent up and bolted with nylon bolts and insulating washers to a 3.18 mm thick aluminum heat sink which is placed over the entire back of the printed circuit (P.C.) card (see Figure 4(a)). The card is then placed in a P.C. board socket mounted behind plug-in locations one and two. All cabling to the plug-ins is soldered to this P.C. board socket. The requirement that the delayed trigger pulse be capable of directly firing a thyratron made the addition of an SCR trigger output necessary. The circuit diagram in Figure 5 shows the finalized design of the pulse shaper and SCR pulse generator. The incoming signal from pins P315-3 and P315-4 of the DD501 is applied to the base of transistor Q_5 . Transistors Q_5 and Q_6 make up a modified Schmidt trigger that is used to generate a large amplitude and stretched pulse. The output of Q_6 is applied to the base of Q_7 connected in a Darlington type circuit to the gate of SCR2. The SCR2 discharges the .05 Mfd disc capacitor into the 50 ohm resistor on the cathode of the SCR2. This is then the desired output pulse. The overall delay of this circuit adds .4 to .5 μ sec to the delay set in by the delay switches on the DD501. SCR2 is selected in order to provide these short delay times. The 60/120 volts D.C. supply required for the SCR2 is generated by a voltage doubler, as shown in Figure 5. Two isolated unused 25 volt A.C. windings are available for each plug-in compartment in the TM506 interface. They are brought out to DD501



*MOUNTED ON TM 506 SPARE FUSE HOLDERS LOCATED ON MAIN INTERFACE BOARD

Figure 3. Schematic Diagram of Clock Circuit and Cable Driver

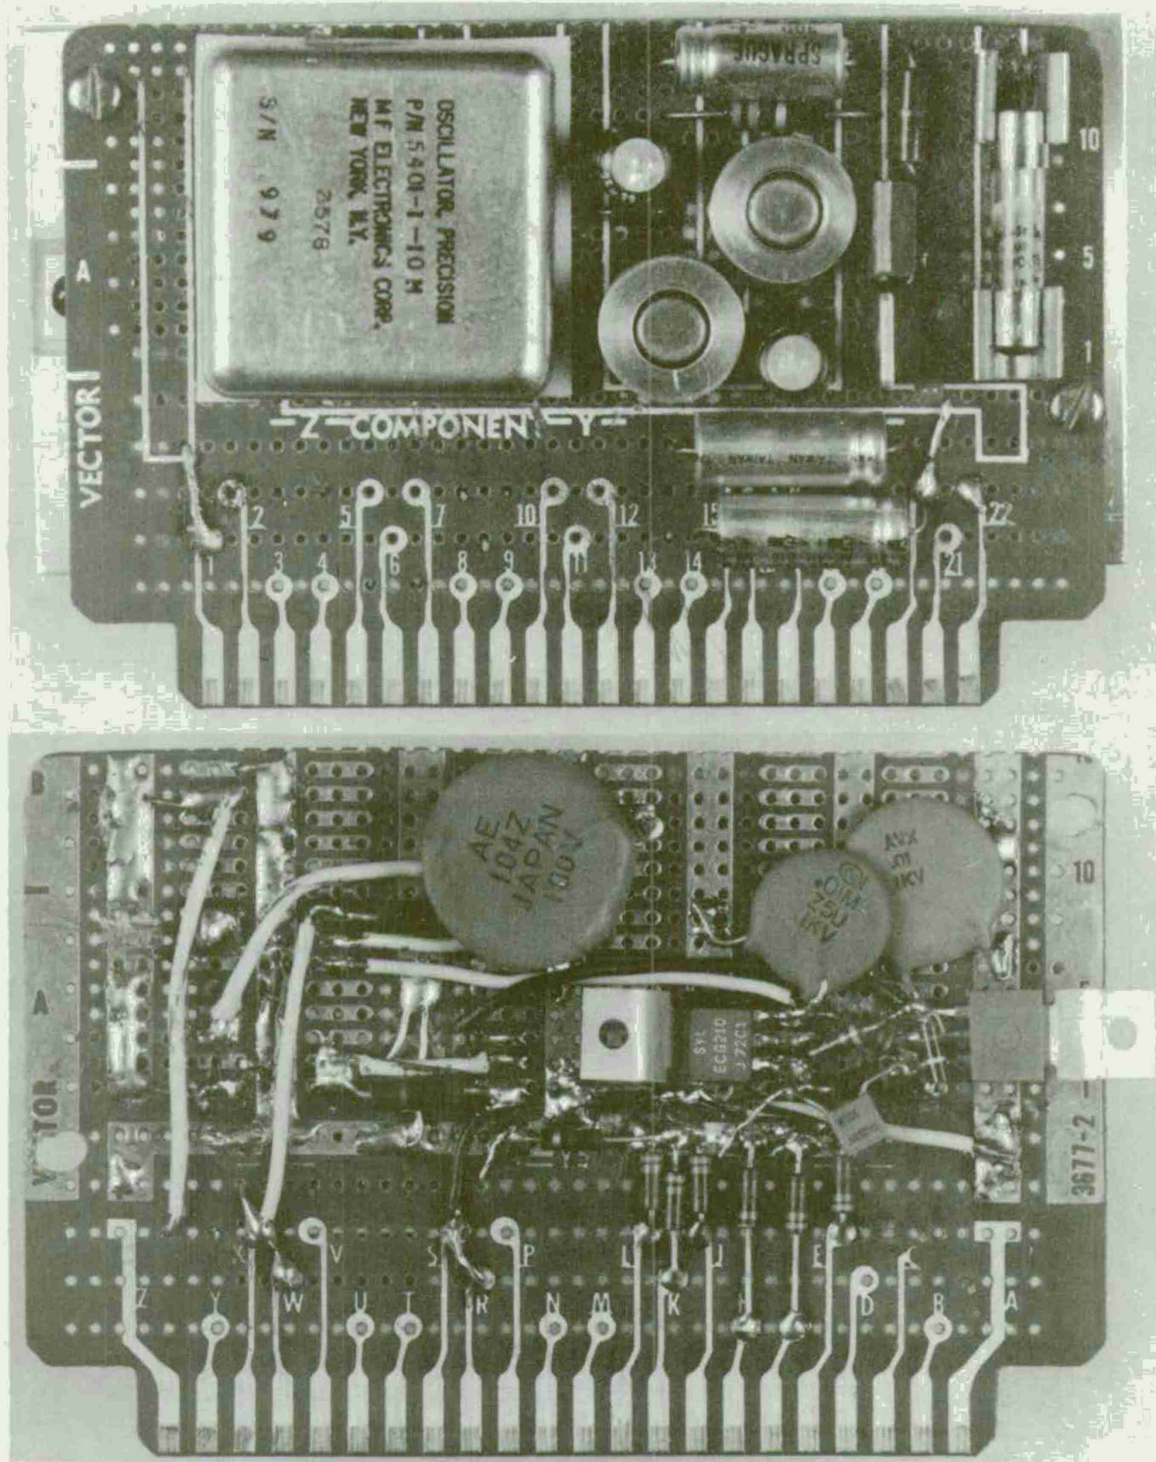


Figure 4. Oscillator Circuit Board
 (A) Component Side
 (B) Circuit Side

Figure 5. Schematic Diagram of Pulse Shaper and Output Driver

user pins and selected by SW1 for either a 60 or 120 volt D.C. output pulse. The physical size of components mounted on the trigger board was kept to a minimum by the use of 1/4 watt resistors and miniature low voltage capacitors. Figure 6 shows the layout of the P.C. board before installation into the DD501. The original connector to pins P315-3 and P315-4 of the DD501 is used to couple to the input of the board. This connector is also used as one of the mounts and standoff for the board. Figure 7 shows the complete installation of the board in the DD501. The board is mounted by a 25 mm standoff and bolt and the above mentioned connector. The wiring to the back interface and front panel is dressed along the bottom of the DD501. Neatness is an absolute necessity since the voltages involved can do extensive damage to the DD501 in case of an accidental short.

The completed six channel system is shown in Figure 8. The entire system occupies only 134 mm of rack space and is completely self-contained. The final specifications from actual measurements are shown in Table I.



Figure 8. Photograph of Completed Six Channel Delay System

TABLE I

Input	-1 to +1 volts, greater than 5ns wide; 1 meg, 20 pF impedance
Output	60 or 120 volts, .1 μ sec risetime adjustable exponential decay
Time Delay Range	5 μ sec to 10,000 μ sec (easily selectable)
Repeatability	.05 μ sec or less after 10 sec

In all tests to date, the units have not only been shown to be reliable but have exhibited an R.F. immunity far better than anticipated. In fact, no R.F. interference from x-ray pulsers or spark cap firing units have been noticed, even using twisted-pair firing lines.

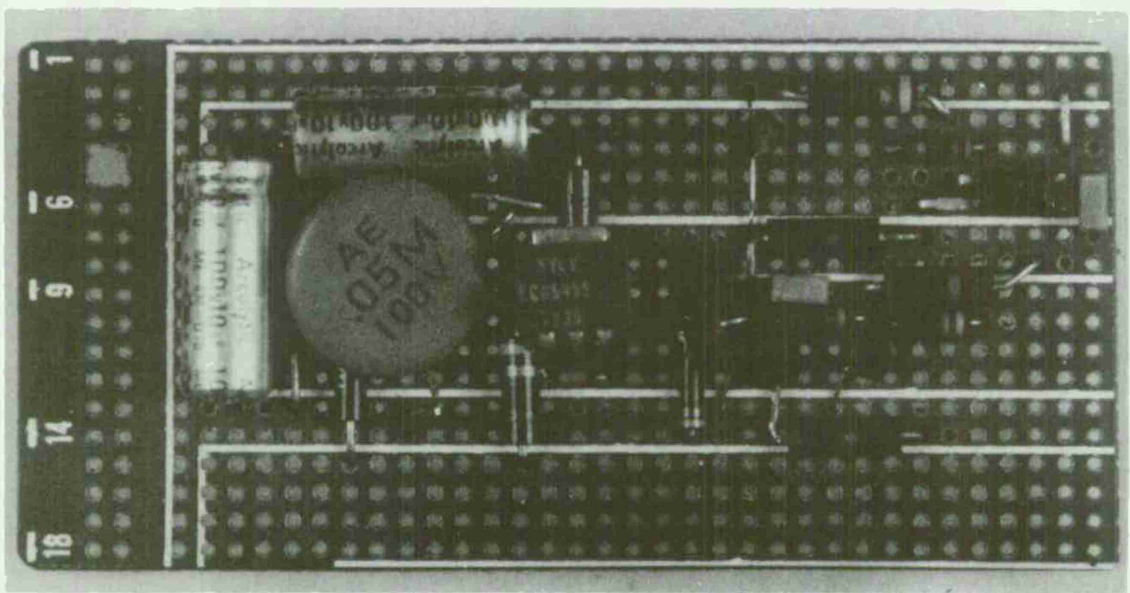


Figure 6. Pulse Shaper and Output Driver Circuit Board

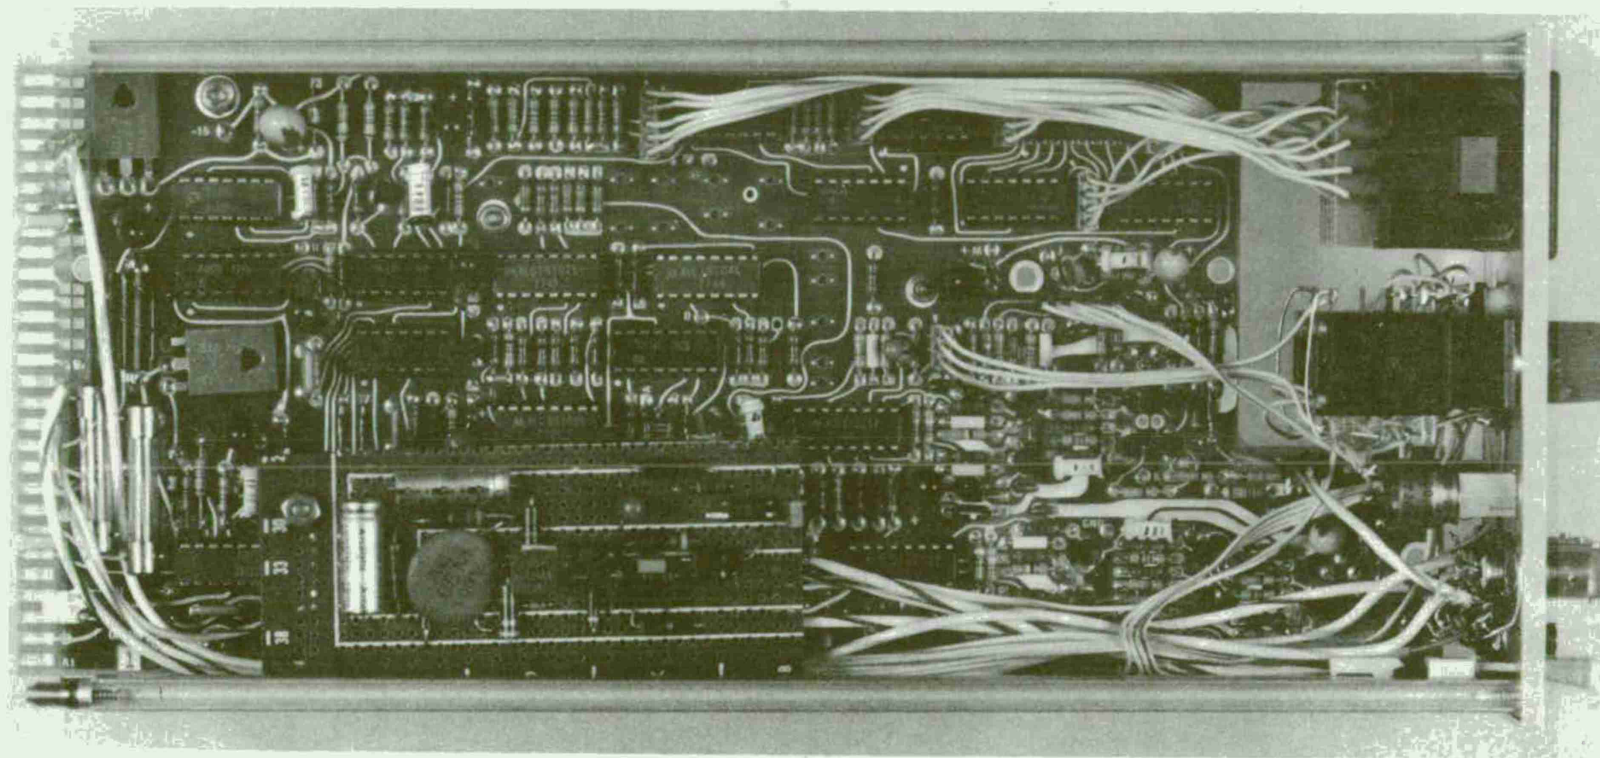


Figure 7. DD501 Events Counter with Pulse Shaper and Output Driver Board Installed

ACKNOWLEDGEMENT

The author wishes to express his sincere appreciation to Mr. Konrad Frank of the Ballistic Research Laboratory for his many suggestions during the development of the circuitry described in this report.

DISTRIBUTION LIST

<u>No. of</u> <u>Copies</u>	<u>Organization</u>	<u>No. of</u> <u>Copies</u>	<u>Organization</u>
12	Commander Defense Technical Info Center ATTN: DDC-DDA Cameron Station Alexandria, VA 22314	1	Commander US Army Electronics Research and Development Command Technical Support Activity ATTN: DELSD-L Fort Monmouth, NJ 07703
1	Commander US Army Materiel Development and Readiness Command ATTN: DRCDMD-ST 5001 Eisenhower Avenue Alexandria, VA 22333	2	Commander US Army Missile Research and Development Command ATTN: DRDMI-R DRDMI-YDL Redstone Arsenal, AL 35809
2	Commander US Army Armament Research and Development Command ATTN: DRDAR-TSS (2 cy) Dover, NJ 07801	1	Commander US Army Tank Automotive Research & Development Cmd ATTN: DRDTA-UL Warren, MI 48090
1	Commander US Army Armament Materiel Readiness Command ATTN: DRSAR-LEP-L, Tech Lib Rock Island, IL 61299	1	Director US Army TRADOC Systems Analysis Activity ATTN: ATAA-SL, Tech Lib White Sands Missile Range NM 88002
1	Commander US Army Aviation Research and Development Command ATTN: DRSAB-E P.O. Box 209 St. Louis, MO 63166	1	Schlumberger Well Services ATTN: C. Aseltine 5000 Gulf Freeway Houston, TX 77023
1	Director US Army Air Mobility Research and Development Laboratory Ames Research Center Moffett Field, CA 94035	<u>Aberdeen Proving Ground</u>	
1	Commander US Army Communications Rsch and Development Command ATTN: DRDCO-PPA-SA Fort Monmouth, NJ 07703	Dir, USAMSAA ATTN: DRXSY-D DRXSY-MP, H. Cohen Cdr, USATECOM ATTN: DRSTE-TO-F Dir, Wpns Sys Concepts Team, Bldg. E3516, EA ATTN: DRDAR-ACW	

USER EVALUATION OF REPORT

Please take a few minutes to answer the questions below; tear out this sheet and return it to Director, US Army Ballistic Research Laboratory, ARRADCOM, ATTN: DRDAR-TSB, Aberdeen Proving Ground, Maryland 21005. Your comments will provide us with information for improving future reports.

1. BRL Report Number _____

2. Does this report satisfy a need? (Comment on purpose, related project, or other area of interest for which report will be used.)

3. How, specifically, is the report being used? (Information source, design data or procedure, management procedure, source of ideas, etc.) _____

4. Has the information in this report led to any quantitative savings as far as man-hours/contract dollars saved, operating costs avoided, efficiencies achieved, etc.? If so, please elaborate.

5. General Comments (Indicate what you think should be changed to make this report and future reports of this type more responsive to your needs, more usable, improve readability, etc.) _____

6. If you would like to be contacted by the personnel who prepared this report to raise specific questions or discuss the topic, please fill in the following information.

Name: _____

Telephone Number: _____

Organization Address: _____

